





ZirChrom®

Technical Bulletin #251

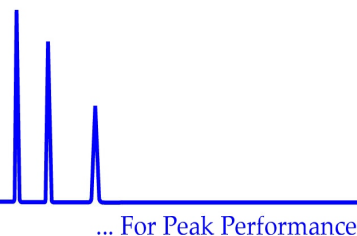

Separation of Progesterone Steroids

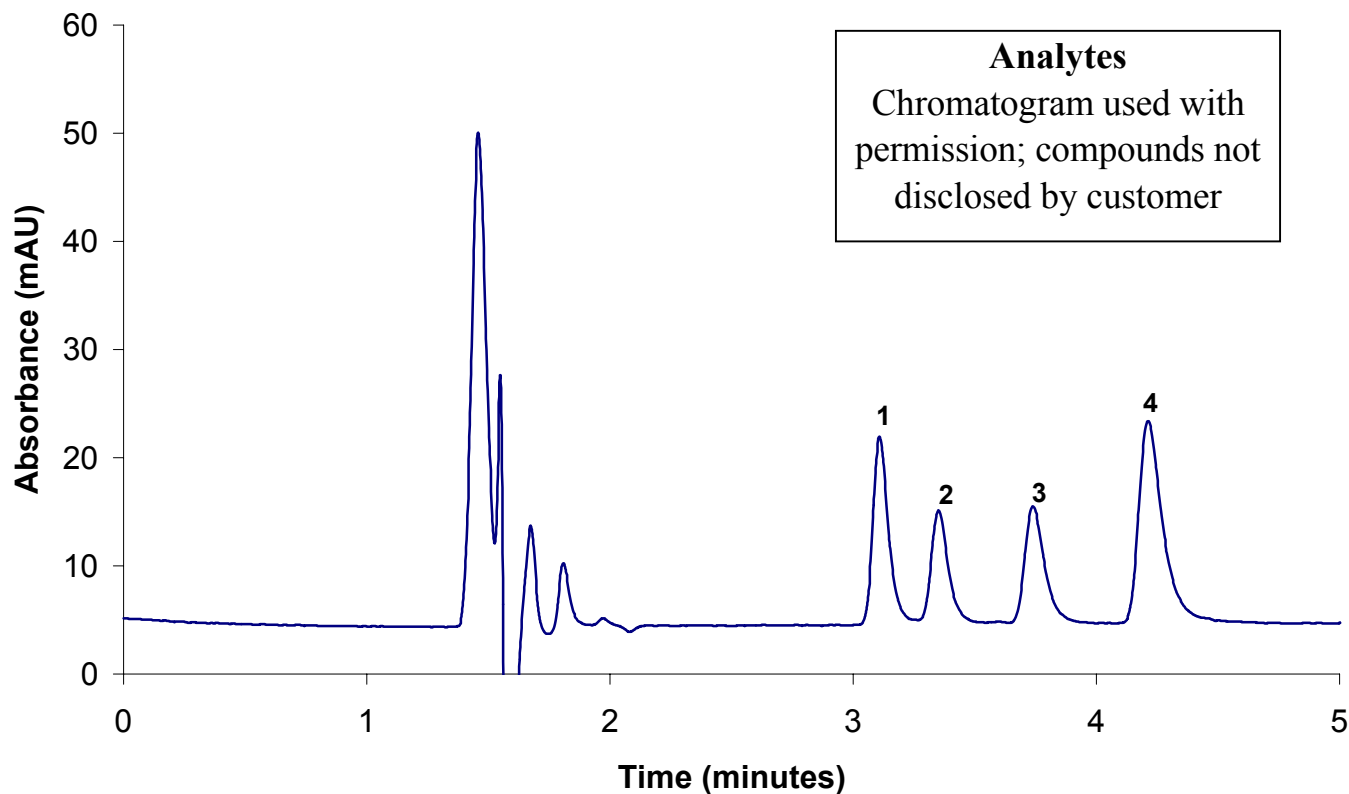

LC Conditions

Column: **DIAMOND BOND™** 18, 100 × 4.6 mm

Mobile Phase: 37.5/27.5/35 A/B/C

A: ACN

B: THF

C: Water

Flow rate: 1.0 mL/min.

Temperature: 75 °C

Injection volume: 5 µL

Detection: 254 nm

